


## Notes and Instructions for the CPPI Air Bearing LVDT Unit



1. Probe should be held using pressure as uniform as possible around circumference of body (A), avoiding deflection-causing pressure points.
2. Brass connector is supplied for use with the stylus retraction port (B).
3. **Operate only clean, dry air at 60psi (C).**
4. Adjust stylus force using supplied allen wrench and rear needle valve (D).
5. Contact CPPI before disassembling unit. (Warranty void if unit opened.)

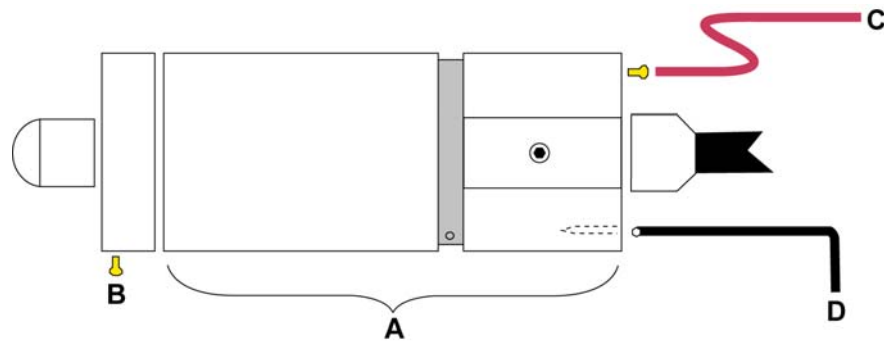